


New calibration settings have been measured.  
Tap the screen to register saved data.  
Wait for 30 seconds to cancel saved data and keep the current setting.

Time limit : 29 sec

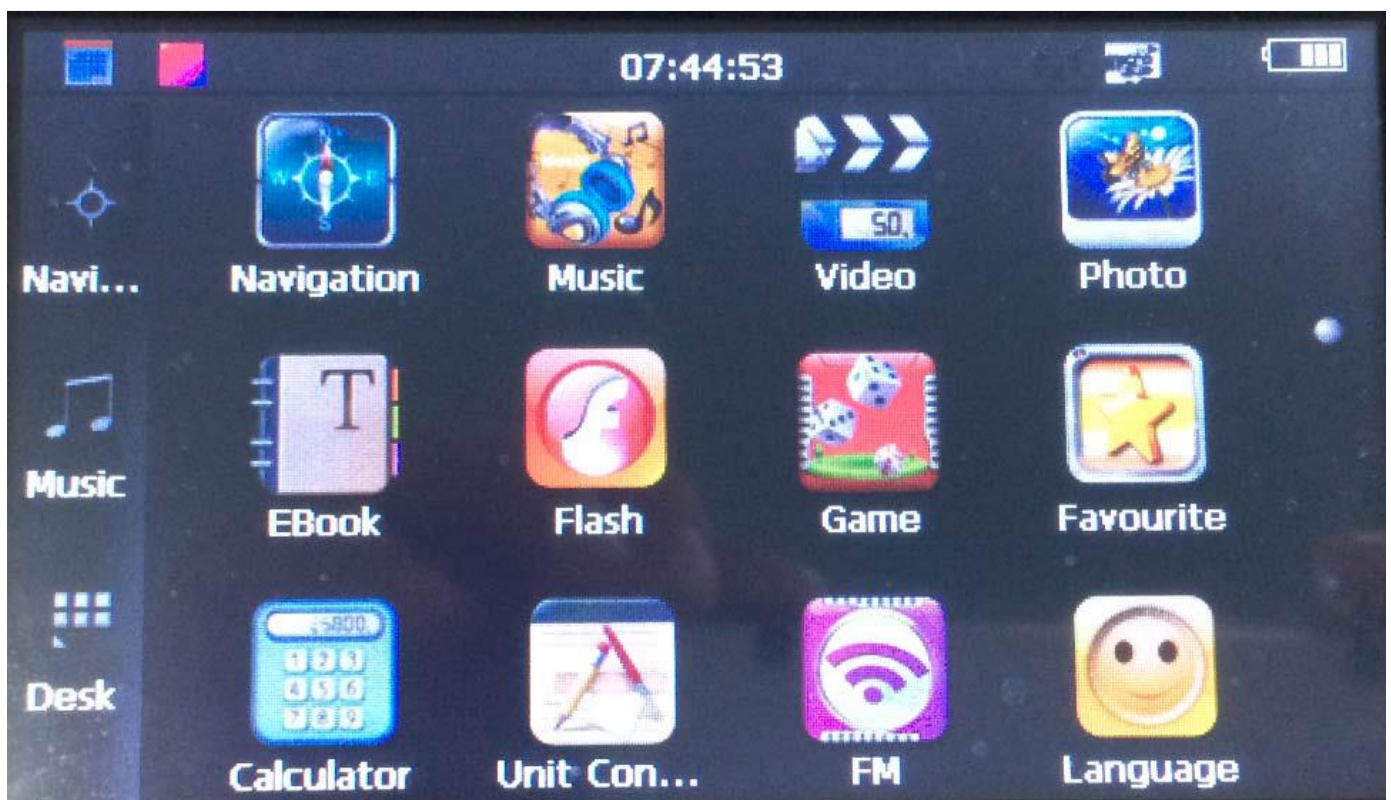

**Aktualizacja zakończona, dziękujemy za wykonanie procedury**